


An on-site dosimetry audit for high-energy electron beams

NEDERLANDSE COMMISSIE VOOR STRALINGSDOSIMETRIE

**Report 29 of the Netherlands Commission on Radiation Dosimetry
October 2018**

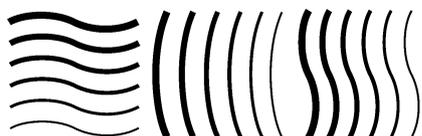


**Netherlands Commission on Radiation Dosimetry
Subcommittee 'Audit for high-energy electron beams'
October 2018**

An on-site dosimetry audit for high-energy electron beams

NEDERLANDSE COMMISSIE VOOR STRALINGSDOSIMETRIE
Report 29 of the Netherlands Commission on Radiation Dosimetry

Authors

Leon de Prez
Stan Heukelom
Bartel Jansen
Wim Jansen
Elfried Kok
Thijs Perik
Jacco de Pooter
Frits Wittkämper (Chairman)

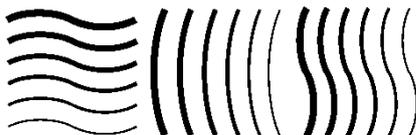

Netherlands Commission on Radiation Dosimetry
Subcommittee 'Audit for high-energy electron beams'
October 2018

Disclaimer regarding NCS reports

The NCS frequently publishes reports for fellow professionals in which recommendations are given for various quality control procedures or otherwise. The members of the NCS board and the members of the concerning subcommittee do not claim any authority exceeding that of their professional expertise. Responsibility on how the NCS recommendations are implemented lies with the user, taking into account the practice in his/her institution.

Certain commercial equipment, instruments, or materials are identified in this report in order to specify the experimental procedure adequately. Such identification does not imply recommendation or endorsement, nor that the materials or equipment identified are necessarily the best available for the purpose.

Preface

The Nederlandse Commissie voor Stralingsdosimetrie (NCS, Netherlands Commission on Radiation Dosimetry, <http://www.radiationdosimetry.org>) was officially established on 3 September 1982 with the aim of promoting the appropriate use of dosimetry of ionizing radiation both for scientific research and practical applications. The NCS is chaired by a board of scientists, installed upon the suggestion of the supporting societies, including the Nederlandse Vereniging voor Radiotherapie en Oncologie (Netherlands Society for Radiotherapy and Oncology), the Nederlandse Vereniging voor Nucleaire Geneeskunde (Dutch Society of Nuclear Medicine), the Nederlandse Vereniging voor Klinische Fysica (Dutch Society for Medical Physics), the Nederlandse Vereniging voor Radiobiologie (Netherlands Radiobiological Society), the Nederlandse Vereniging voor Stralingshygiëne (Netherlands Society for Radiological Protection), the Nederlandse Vereniging voor Medische Beeldvorming en Radiotherapie (Dutch Society for Medical Imaging and Radiotherapy), the Nederlandse Vereniging van Klinisch Fysisch Medewerkers (Dutch Society for Medical Physics Engineers), the Nederlandse Vereniging voor Radiologie (Radiological Society of the Netherlands) and the Belgische Vereniging voor Ziekenhuisfysici/Société Belge des Physiciens des Hôpitaux (Belgian Hospital Physicists Association). To pursue its aims, the NCS accomplishes the following tasks: participation in dosimetry standardisation and promotion of dosimetry intercomparisons, drafting of dosimetry protocols, collection and evaluation of physical data related to dosimetry. Furthermore, the commission shall maintain or establish links with national and international organisations concerned with ionizing radiation and promulgate information on new developments in the field of radiation dosimetry.

Current members of the board of the NCS

J.B. van de Kamer, Chairman
T.W.M. Grimbergen, Vice-Chairman
J.A. de Pooter, Secretary
J.M.J. Hermans, Treasurer
A. Rijnders
N. De Graaf
F.W. Wittkämper
M.K. de Fluiter-Zeeman
J.R. de Jong
P. Sminia
N.A.P. Franken

An on-site dosimetry audit for high-energy electron beams

Members of the subcommittee:

Frits Wittkämper

Stan Heukelom

Bartel Jansen

Wim Jansen

Elfried Kok

Thijs Perik

Jacco de Pooter (Advisor)

Leon de Prez

NCS, Delft, the Netherlands

For more information on NCS Reports, see <http://radiationdosimetry.org>

Summary

The NCS code of practice for high-energy photon and electron beams [1] has currently been implemented in most of the Dutch and Belgium radiotherapy institutes. Recently, the NCS performed a photon dosimetry audit at a large number of Dutch and Belgium radiotherapy departments [2] that has been continued as a VSL dosimetry service. In order to implement an electron audit rather quickly and efficiently, the NCS decided to establish a small audit group amongst four radiotherapy departments which already implemented the NCS 18 [1] code of practice for electron beams. The goal of this subcommittee was to establish a dosimetry audit for absorbed dose to water, D_w , in electron beams.

The subject of the audit is the determination of absorbed dose to water, D_w in cGy, at reference depth, z_{ref} , as well as the beam quality specifier, $R_{50,dos}$ in cm, in high-energy electron beams in the participant's accelerator facility as performed by local staff. The audit results are expressed as an E_n -score [3], where the outcome of the audit is either 'satisfactory' when $|E_n| \leq 1.0$ or 'unsatisfactory' when $|E_n| > 1.0$.

The so called 'reference values' of $R_{50,dos}$ and D_w as measured by the audit team were performed according to NCS 18 [1]. Measurements of D_w and the percentage depth ionization curve (PDI) to obtain the beam quality, $R_{50,dos}$, were performed with a plane-parallel ionization chamber. D_w was based on a plane-parallel chamber's ^{60}Co calibration. Additionally, if an electron energy with $R_{50,dos} > 7$ cm was available, a cross-calibration of the plane-parallel chamber against a Farmer type chamber was performed.

The expanded uncertainty for $R_{50,dos}$ was estimated to be 0.14 cm ($k=2$). The relative expanded uncertainty in D_w at z_{ref} with a plane-parallel chamber calibrated in ^{60}Co was estimated to be 3.6 % ($k=2$).

For the uncertainty in the D_w audit result, Δ_{D_w} , correlations between the measured values by audit team and the participant were taken into account. This resulted in an estimated relative uncertainty for Δ_{D_w} of 2.4 %. The uncertainty in the audit result for $R_{50,dos}$ was estimated to be 0.20 cm.

A total of 15 electron beams were measured in 4 participating institutes. One institute was measured twice, i.e. at the beginning of the audit campaign as an initial test audit and at the end of the audit campaign as an actual audit. Both results have been reported.

All $R_{50,dos}$ audit results, $\Delta_{R_{50,dos}}$ turned out to be satisfactory (i.e. $|E_n| \leq 1.0$) except for one electron beam with an unsatisfactory E_n -score of 1.4. It did not influence the audit result on the D_w measurement and therefore the overall audit result of this participant. All D_w audit results, Δ_{D_w} , turned out to be satisfactory (i.e. $|E_n| \leq 1.0$).

Overall it can be concluded that the audit was implemented successfully. Differences of D_w values between the audit team and the participant were in all cases smaller than 1 % and in most cases smaller than 0.5 % with a relative uncertainty of 2.4 % ($k = 2$). Differences in $R_{50,dos}$ were in all cases smaller than 0.3 cm and in most cases smaller than 0.2 cm with an uncertainty of 0.20 cm. Except for the first (test) audit, D_w values obtained with a plane-parallel chamber calibrated in ^{60}Co and cross-calibrated in a high-energy electron cross-calibration agreed within 0.3 %.

It must be noted that the audit described in this study, has been performed at radiotherapy departments traceable to VSL by applying the same code of practice as the audit team. If this audit would be performed at departments not traceable to VSL or that these departments apply a different dosimetry protocol than the audit team, the uncertainties reported in this study do not apply.

This NCS subcommittee had its kick-off meeting at 2 February 2015.

Contents

1	Introduction	9
1.1	History.....	9
1.2	The need for dosimetry audits	9
1.3	Goal of the NCS subcommittee 'Electron Audit'	9
2	Audit protocol	11
2.1	Subject and measured quantities	11
2.2	Reporting of the measurements and audit results	11
2.3	Measurement conditions	12
3	Measurement equipment and methods	13
3.1	General measurement procedure.....	13
3.2	Water phantom and positioning.....	13
3.3	Measurement of $R_{50,dos}$ and determination of z_{ref}	14
3.4	Measurement of percentage depth ionization curve, PDI	14
3.5	D_w measurement.....	15
3.6	Calibration coefficient of the plane-parallel chamber in beam quality Q, $N_{D,w,Q}^{PP}$	15
3.6.1	Plane-parallel chamber calibrated in ^{60}Co	16
3.6.2	Plane-parallel chamber cross-calibrated in a high-energy electron beam.....	16
3.7	Electrometer and ionization chamber correction factors	17
4	Uncertainties	19
4.1	Uncertainties on the reference values	19
4.1.1	Uncertainty in $R_{50,dos}$ and z_{ref}	19
4.1.2	Uncertainty in a charge measurement at a depth of z_{ref}	20
4.1.3	Uncertainty in D_w	21
4.2	Uncertainties in the audit results.....	23
4.2.1	Uncertainty in audit result for $R_{50,dos}$, $\Delta_{R,50,dos}$	23
4.2.2	Uncertainty in audit result for D_w , $\Delta_{\%,D,w}$	23
5	Results.....	26
5.1	Reference and participants' values.....	26
5.2	Audit results	26
6	Discussion and conclusion	30
7	Acknowledgements	31
	References.....	32

1 Introduction

1.1 History

In 2008 the Netherlands Commission on Radiation Dosimetry (NCS) issued a new code of practice for high-energy photon and electron beams based on absorbed dose to water standards, NCS 18 [1]. The new code of practice (CoP) replaced the air kerma based CoP described in NCS reports 2 and 5 [4,5]. NCS 18 is currently adopted or being implemented in the majority of the Dutch and Belgium radiotherapy departments.

1.2 The need for dosimetry audits

An external dosimetry audit after introducing a new dosimetry protocol or on a periodical basis is a powerful quality assurance instrument for radiotherapy departments. Therefore, the NCS decided to install a subcommittee with the aim to develop a reference dosimetry audit for electron beams to enable independent validation of the implementation of NCS 18 for electron beams. After development of the method and performing the audit, the audit method is transferred to VSL, the Dutch national metrology institute, which will offer audits for electron beams to users upon request. A similar approach was applied to set-up the photon beam audit, described in NCS report 23 [2], where the measurement protocol and procedures of the NCS subcommittee were adopted by VSL. This approach assures that the VSL adopted audit service is in accordance with the needs of radiotherapy departments. To reduce workload and enhance efficiency of the subcommittee it was decided to perform the audit for a relatively small group of radiotherapy departments (Table 1.1), which already adopted the NCS 18 [1] code of practice for their electron dosimetry.

Table 1.1: Participating radiotherapy departments.

name	short	city	site location
The Netherlands Cancer Institute	AVL	Amsterdam	Amsterdam
Leiden University Medical Center	LUMC	Leiden	Leiden
Reinier de Graaf	RdG	Delft	Delft
VU University Medical Center	VUmc	Amsterdam	Hoorn

1.3 Goal of the NCS subcommittee 'Electron Audit'

The goal of the NCS subcommittee 'Electron Audit' is to establish an electron dosimetry audit for absorbed dose to water, D_w , and electron beam quality, $R_{50,dos}$, under defined reference conditions. Table 1.2 summarizes the electron beams chosen for testing the audit protocol

and measurements. The audit results are based on the $R_{50,dos}$, and D_w at reference depth, Z_{ref} .

The visit at the first radiotherapy department was considered a 'test' audit in order to become familiar with the audit equipment in an electron dosimetry setting. The audit at this radiotherapy department was repeated at the end of the measurement campaign as the actual audit for this radiotherapy department.

Table 1.2: Overview of the electron beams. Here SSD is the Source Detector Distance and 'isoc' refers to the beam's iso-centre².

participant	linear accelerator type	nominal energies /MeV	SSD /cm	field size at isoc /cm ²
AVL	Elekta Synergy (MLCi)	6; 12; 18	95	10.5 × 10.5
RdG	Elekta Synergy (Agility)	4; 10; 15	100	10.5 × 10.5
VUmc	Varian TrueBeam	6; 9; 22	100	10 × 10
LUMC	Elekta Synergy (MLCi)	4; 12; 4HDRE ¹	100	10.5 × 10.5 / 42 × 42 ¹
AVL	Elekta Synergy (MLCi)	6; 12; 18	95	10.5 × 10.5

¹ High Dose Rate Electron beam (HDRE) with field size of 42 × 42 cm², which is larger than the surface of the audit phantom.

² The field size is determined by the accelerator applicator. For Elekta accelerators the field size is defined at 95 cm, thus for a 10 × 10 cm² applicator the field size in the iso-centre is 10.5 × 10.5 cm². For Varian accelerators the field size is defined at 100 cm, resulting in a field size in the iso-centre of 10 × 10 cm².

2 Audit protocol

2.1 Subject and measured quantities

The subject of the audit is the determination of absorbed dose to water, D_w in cGy, at reference depth, z_{ref} , as well as the beam quality specifier, $R_{50,dos}$ in cm, in high-energy electron beams. The participant's staff performs measurements according to local dosimetry procedures and using local equipment. The NCS-team performs measurements according to the procedures described in this report and using the NCS-team's equipment. The NCS measurements are referred to as the audit's 'reference values'. Participant and NCS-team perform D_w and $R_{50,dos}$ measurements on the same day.

2.2 Reporting of the measurements and audit results

The participant's values and reference values are part of the audit report. It is unusual for radiotherapy departments to report uncertainties. NCS-team and participant perform their dosimetry at the same reference conditions and with similar, calibrated equipment. Therefore, it is unlikely that the participant's uncertainties are smaller than those of the NCS-team. For reasons of simplicity, it is assumed that the uncertainties on the participant's values are at least that of the uncertainty on the reference value.

The audit is established as a comparison between the measured value, x , by the participating institute and measured reference value, X , by the NCS audit team. The evaluation of the comparison is expressed as an, E_n -score [3]:

$$E_n = \frac{\Delta}{U_\Delta} \quad (1)$$

where Δ is the difference between the participant's value, x , and the reference value, X :

$$\Delta = x - X \quad (2)$$

- x is the measured value by the participant;
- X is the assigned reference value, measured by the NCS audit team;
- U_Δ is the expanded uncertainty ($k = 2$) on the difference, Δ .

The outcome of the audit, expressed as E_n , in accordance with [3], is either:

'satisfactory' when $|E_n| \leq 1.0$

or

'unsatisfactory' when $|E_n| > 1.0$

The audit result in the $R_{50,dos}$ (section 3.3) is expressed as an absolute value in the unit cm:

$$\Delta_{R_{50,dos}} = R_{50,dos} - R_{50,dos,ref} \quad (3)$$

The audit result in the D_w measurement (see section 3.5) is expressed as a relative value, expressed in:

$$\Delta_{D_w} = \frac{D_w - D_{w,ref}}{D_{w,ref}} \quad (4)$$

Combining equations (1), (3) and (4), the audit results are evaluated using a normalized error, E_n -score:

$$E_{n,R_{50,dos}} = \frac{\Delta_{R_{50,dos}}}{U_{\Delta_{R_{50,dos}}}} \quad (5)$$

and

$$E_{n,D_w} = \frac{\Delta_{D_w}}{U_{\Delta_{D_w}}} \quad (6)$$

where, $U_{\Delta_{R_{50,dos}}}$, in cm, is the expanded uncertainty for the audit result in $R_{50,dos}$. $U_{\Delta_{D_w}}$, in %, is the expanded relative uncertainty on the audit result for D_w . In this study the overall outcome of the audit is only based on the E_n -score for the D_w measurement.

2.3 Measurement conditions

The reference measurements are carried out according to NCS 18 [1]. The reference measurements by the NCS audit team are performed at the same SSD (Source Surface Distance) as the participant's measurements. The D_w measurements performed by both the NCS audit team and the participant are performed at the same number of accelerator monitor units. The following reference conditions apply:

- source surface distance, SSD: 95 cm or 100 cm (depending on participant's SSD);
- depth in water, z_{ref} : based on $R_{50,dos}$ according to equation (8) in section 3.3;
- Field size at iso-center: $\geq 10 \times 10 \text{ cm}^2$, applied according to Table 1.2;
- Water phantom: $\geq 30 \times 30 \times 30 \text{ cm}^3$ (see section 3.2).

The required ambient conditions for the measurements are:

- phantom (water) temperature, T_w : $16 \text{ }^\circ\text{C} < T_w < 26 \text{ }^\circ\text{C}$;
- room temperature, T_{room} : $(T_w - 4 \text{ }^\circ\text{C}) < T_{room} < (T_w + 4 \text{ }^\circ\text{C})$;
- ambient pressure, p : atmospheric;
- relative humidity, RH%: 20 % - 80 %.

3 Measurement equipment and methods

3.1 General measurement procedure

The general audit procedure is as follows. After setting up the audit equipment and aligning the water phantom, as described in section 3.2, percentage depth ionization (PDI) curves and D_w are measured, as described in sections 3.3 and 3.5 respectively. For practical reasons it was decided to use the same plane-parallel chamber for both the D_w and the PDI measurements. The D_w measurement with the plane-parallel chamber is traceable to primary standards via the chamber's ^{60}Co calibration. If an electron beam with beam quality $R_{50,\text{dos}} > 7$ cm is part of the audit, a cross-calibration of the plan-parallel against a Farmer-type chamber, as described in section 3.6.2, is done immediately following the D_w measurements in the highest energy. After the NCS-team performs the audit measurements, the participant is given time to perform their absolute dosimetry for the same electron energies. On the day of the audit only D_w is measured by the participant. However, in this study some participants also measured $R_{50,\text{dos}}$. The audit is finalized by a repetition of D_w measurement by the NCS-team. The complete electron audit measurement takes between 4 and 6 hours.

3.2 Water phantom and positioning

A water phantom with outer dimensions of $32 \times 37 \times 32$ cm³ ($L \times W \times H$) and wall thickness of 2 cm is used by NCS-team (PTW MP1 T41025). The phantom tank is equipped with an automated vertical translation stage and control unit (PTW TBA). A custom made PMMA (polymethyl methacrylate) bridge is used to mount ionization chambers on the translation stage's vertical carriage by means of the PTW mounting system. The purpose of the bridge is to place the chamber in the centre of the phantom and to minimize beam scatter as a result of the beam hitting metal parts of the translation stage.

The water phantom is placed on top of the patient couch. The couch is used to move the phantom up and down as desired. A calibrated metal ruler attached to the side of the water phantom is used to adjust the patient treatment couch' displacement in vertical direction in relation to the room laser in a similar way as described by Perik et al. [2]. Note that the displacement indicator of the couch is not used in order to avoid possible displacement errors.

3.3 Measurement of $R_{50,dos}$ and determination of z_{ref}

$R_{50,dos}$ is determined by means of the measured percentage dose ionization (PDI) curves, described in section 3.4. $R_{50,dos}$ is based on the distance between the water surface and the point beyond the dose maximum, where the PDI has a value of 50 %, $R_{50,ion}$ according to [1]:

$$R_{50,dos} = 1.029 R_{50,ion} - 0.06 \text{ cm} \quad \text{for } R_{50,ion} \leq 10 \text{ cm}$$

$$R_{50,dos} = 1.059 R_{50,ion} - 0.37 \text{ cm} \quad \text{for } R_{50,ion} > 10 \text{ cm}$$
(7)

Additionally, the $R_{50,dos}$ is determined from the percentage depth dose curve (PDD) after conversion of the PDI to a PDD. This is done by multiplying the PDI with the mass stopping power ratios $s_{w,air}$ according to the method described by Andreo et al. [6]. In this study, $R_{50,dos}$ determined with both methods (based on PDI conversion and based applied in according to equation (7) have been compared. Differences were always smaller than 0.03 cm and therefor considered insignificant. $R_{50,dos}$ is used to determine the reference measurement depth for the D_w measurements, z_{ref} , and determined according to [1]:

$$z_{ref} = 0.6 R_{50,dos} - 0.1 \text{ cm}$$
(8)

3.4 Measurement of percentage depth ionization curve, PDI

The PDI is measured with the plane-parallel ionization chamber based on the position of its effective point of measurement (EPOM), for the used plane-parallel ionization chamber the EPOM is 0.112 cm behind the chambers' front surface. NCS 18 [1] recommends to use a $20 \times 20 \text{ cm}^2$ field at the high-energy electron beams ($R_{50,dos} > 7 \text{ cm}$) because of possible insufficient scatter equilibrium at the central axis [7]. However, all PDI measurements are performed with a beam size close to $10 \times 10 \text{ cm}^2$ (except for the 4HDRE beam at LUMC). The reason for this is that the applicator tray, with the monitor ionization chamber attached to it, doesn't need to be changed during the measurements of the PDI curves, i.e. the curves can be measured without interruption. In order to verify the validity of this method, PDI curves were measured in the highest energy beam (22 MeV at VUmc) both with beam sizes of $10 \times 10 \text{ cm}^2$ and $20 \times 20 \text{ cm}^2$. The measured PDI curves were converted to $R_{50,dos}$ using equation (7). In this study the difference between $R_{50,dos}$ in a $10 \times 10 \text{ cm}^2$ field and in a $20 \times 20 \text{ cm}^2$ field was found to be smaller than 0.04 cm and therefore considered negligible for beams up to 22 MeV.

Corrections for chamber polarity, k_{pol} , and irradiation of the stem, k_{stem} , with depth have not been applied. With respect to k_{pol} , it is assumed that it's variation with depth, i.e. between $R_{100,ion}$ and $R_{50,ion}$ is negligible [8]. Additionally, the variation in stem effect with depth is considered to be insignificant and close to the PDD 50 % point for all energies.

Recombination varies as a function of depth, due to a varying dose per pulse. Therefore, the measured charge is corrected for recombination as a function of depth. This is done by the assumption that the recombination effect, determined at z_{ref} with the two-voltage method recommended by NCS 18 [1], is dominated by volume recombination (neglecting initial recombination) and thus proportional to the depth dose relative to D_w at z_{ref} .

The NCS 18 [1] formalism is used to convert the measured $R_{50,ion}$ value, uncorrected for recombination, to z_{ref} at which D_w is measured. The recombination correction is subsequently measured at z_{ref} according to the method described by Weinhaus and Meli [9], by reducing the chamber voltage by a factor 4. Hence, the reference depth, z_{ref} at which the actual D_w measurement takes place is determined with $R_{50,ion}$ uncorrected for k_s . This causes a small error of up to 0.01 cm in the actual depth of the chamber in water compared to the desired z_{ref} and has been accounted for in the uncertainty.

For the measurement of the PDIs an independent monitor ionization chamber (Semiflex PTW 31013) is used to normalize for beam output fluctuations. This monitor chamber is mounted on the applicator tray at the edge of the beam. Its sensitive volume is completely inside the electron beam but positioned such that it doesn't influence the reading of the detector. The plane-parallel and monitor ionization chambers are connected to a dual channel electrometer and are read out simultaneously while the translation stage is moved in vertical direction upwards. Data-acquisition of PDI is performed automatically by means of commercially available software (PTW MEPHYSTO mc² tbaScan) and the obtained data is analysed in a spreadsheet.

3.5 D_w measurement

The absorbed dose to water, D_w , in electron beam quality, Q , is measured using a waterproof plane-parallel ionization (PTW 34001) chamber connected to a single channel electrometer (PTW UNIDOS T10002) and obtained according to the formalism described in NCS 18 [1]:

$$D_{w,Q} = M_{corr}^{PP} N_{D,w,Q}^{PP} \quad (9)$$

where M_{corr}^{PP} is the corrected electrometer reading (section 3.7) and $N_{D,w,Q}^{PP}$ is the plane-parallel chamber calibration coefficient in beam quality Q (section 3.6).

3.6 Calibration coefficient of the plane-parallel chamber in beam quality Q , $N_{D,w,Q}^{PP}$

The plane-parallel chamber's calibration coefficient in beam quality Q , $N_{D,w,Q}^{PP}$, is based on a ⁶⁰Co calibration, $N_{D,w,Q0}$, with beam quality correction $k_{Q,Q0}^{PP}$. Additionally, a cross-calibration

at a high-energy electron beam with $R_{50,dos} > 7$ cm (when available) against a cylindrical chamber is performed. For the audit result the chamber's ^{60}Co calibration is used.

3.6.1 Plane-parallel chamber calibrated in ^{60}Co

The plane-parallel chamber is calibrated in ^{60}Co with a beam size of 10×10 cm² at a Source Detector Distance (SDD) of 100 cm. The calibration coefficient, $N_{D,w,Q}^{PP}$, in electron beam quality Q is determined according to:

$$N_{D,w,Q}^{PP} = N_{D,w,Q_0}^{PP} k_{Q,Q_0}^{PP} \quad (10)$$

where N_{D,w,Q_0}^{PP} is the ^{60}Co calibration of the plane-parallel ionization chamber and k_{Q,Q_0}^{PP} is the plane-parallel chamber's beam quality dependent ionization chamber correction factor according to equation (11) and Table 2 in NCS 18 [1].

3.6.2 Plane-parallel chamber cross-calibrated in a high-energy electron beam

Optionally, a cross-calibration of the plane-parallel chamber against a Farmer type cylindrical chamber (NE2571) takes place in a high-energy electron beam with beam quality $R_{50,dos} > 7$ cm in the accelerator of the participant (when available). The cross-calibration procedure is followed according to NCS 18 [1] and $N_{D,w,Q}^{PP}$ in beam quality Q is determined according to:

$$N_{D,w,Q}^{PP} = N_{D,w,Q_{cross}}^{PP} k_{Q,Q_{cross}}^{PP} \quad (11)$$

where $N_{D,w,Q_{cross}}^{PP}$ is the plane-parallel chamber's cross-calibration coefficient in a high-energy electron beam with $R_{50,dos} > 7$ cm. $k_{Q,Q_{cross}}^{PP}$ is the ratio of beam quality correction factors for the plane-parallel chamber at beam quality Q and at the cross-calibration quality Q_{cross} , obtained from NCS 18 [1]. The plane-parallel chamber's calibration coefficient in Q_{cross} , $N_{D,w,Q_{cross}}^{PP}$, is determined according to:

$$N_{D,w,Q_{cross}}^{PP} = \frac{M_{Q_{cross}}^{CYL}}{M_{Q_{cross}}^{PP}} N_{D,w,Q_0}^{CYL} k_{Q_{cross},Q_0}^{CYL} \quad (12)$$

Here, N_{D,w,Q_0}^{CYL} is the ^{60}Co calibration coefficient of the Farmer type cylindrical ionization chamber and $k_{Q,Q_{cross}}^{CYL}$ is the cylindrical chamber's beam quality correction factor according to equation (14) and Table 2 in NCS 18 [1]. $M_{Q_{cross}}^{CYL}$ and $M_{Q_{cross}}^{PP}$ are the corrected electrometer

readings, later indicated as M_{corr} in equation (13), with the respective chambers positioned at z_{ref} for a specified number of accelerator monitor units.

The plane-parallel and the cylindrical ionization chamber are subsequently connected to a single channel electrometer (PTW UNIDOS T10002), relying on the short-term stability of the accelerator monitor. The cylindrical ionization chamber is placed inside a VSL made waterproof PMMA sleeve with a wall thickness of 1 mm. A thin latex tube is impermeably connected to the waterproof sleeve in order to keep the cylindrical ionization chamber and its cable dry when submerged.

During the cross-calibration procedure both ionization chambers are positioned with their effective point of measurement (EPOM) at a depth of z_{ref} at the central axis of the beam. For the PTW Roos (PTW 34001) plane-parallel chamber the EPOM this is 0.112 cm from the front surface of the ionization chamber according to the manufacturer's documentation. For the cylindrical chamber the EPOM is at $0.5 \times$ the radius of the chamber central axis (i.e. +0.158 cm for the NE2571 ionization chamber used in this study), also explained and illustrated in Figure 3 in NCS 18 [1]. This means that the centre of the cylindrical chamber is positioned 0.158 cm of the geometrical centre away from the accelerator focus. The bias voltages of the plane-parallel and cylindrical chamber are set to respectively +200 V and +300 V.

3.7 Electrometer and ionization chamber correction factors

The corrected electrometer reading for the plane-parallel and the Farmer type cylindrical chamber, M_{corr} (to improve readability the subscript 'corr' was omitted in the previous sections), is obtained according to:

$$M_{\text{corr}} = M k_{\text{elec}} k_{pT} k_s k_{\text{pol}}^+ \quad (13)$$

where the electrometer reading, M , is corrected for:

- electrometer calibration, k_{elec} (electrometer and ionization chamber are calibrated as separate instruments, i.e. not as a dosimetry system);
- air cavity density compared to reference air density based on the ambient pressure and temperature, k_{pT} ;
- incomplete charge collection due to recombination, k_s [9];
- chamber polarity, k_{pol}^+ (+ indicates an applied positive bias voltage).

All correction factors are determined according to generally accepted methods such as described in NCS 18 [1].

A correction for air cavity density, k_{pT} , compared to reference air density (20 °C and atmospheric pressure of 101.325 kPa) is applied since the used ionization chambers are open

to ambient air. The water temperature, used for k_{pT} , is measured with a thermometer (Omega HH41) with its thermistor positioned inside a stainless-steel waterproof sleeve at the same depth as the ionization chamber just outside the radiation field. The atmospheric pressure is determined inside the accelerator room (Vaisala PTU300).

Since the chamber's ^{60}Co calibration coefficients were corrected for polarity effect, in the electron beams a correction for chamber polarity, k_{pol}^+ is applied based on a chamber positive bias voltage.

The ambient temperature and relative humidity are measured inside the accelerator room (Vaisala PTU300) in order to verify that the air temperature is not outside its desired range. A correction for air relative humidity, k_h , is not applied since the chamber calibration coefficients have been measured at a relative humidity in the range between 20 % and 80 % for which the ionization chamber response varies < 0.1 % [10].

Furthermore, no correction is applied for dose averaging over the chamber volume caused by beam radial non-uniformity, k_{rn} , as it is a small effect regarding electron beam profiles used in this study.

4 Uncertainties

4.1 Uncertainties on the reference values

The reported expanded uncertainty, U , on the measured reference values is based on the standard uncertainty, u , multiplied by a coverage factor $k = 2$, which for a normal distribution corresponds to a coverage probability of approximately 95%, unless mentioned otherwise. The standard uncertainty has been determined in accordance with the GUM 'Evaluation of measurement data - Guide to the Expression of Uncertainty in Measurement' [11]. Uncertainties are expressed in 2 significant digits with a minimum resolution of 0.01 % or 0.01 cm.

4.1.1 Uncertainty in $R_{50,dos}$ and z_{ref}

Table 4.1 gives the uncertainty budget for determination of $R_{50,dos}$ in cm. Where needed, relative uncertainty contributions due to charge measurements have been converted to cm with a sensitivity coefficient of $0.03 \text{ cm } \%^{-1}$ based on a minimum PDD of $-4 \% \text{ mm}^{-1}$ at $R_{50,dos}$ at 22 MeV. All uncertainty contributions are of type B and are applicable for the percentage depth ionization curves (PDIs) described in section 3.4. The uncertainty budget for $R_{50,dos}$ is based on a PDI measured with a Roos ionization chamber. Uncertainty contributions are added with respect to the conversion from PDI to PDD based on a variation of stopping power ratios, $s_{w,air}$, and positioning of the chamber. The standard uncertainty in determination of $R_{50,dos}$ is estimated to be 0.07 cm (quadratic sum of two 0.05 cm uncertainties). The associated standard uncertainty in z_{ref} due to $R_{50,dos}$ is based on the uncertainty of $R_{50,dos}$ and its conversion with a corresponding sensitivity coefficient of 0.6 estimated to be 0.04 cm.

Table 4.1: Uncertainty budget for determination of $R_{50,dos}$ in cm. All uncertainty contributions are of type B. Uncertainties in charge measurements are converted to depth with a sensitivity coefficient of $0.03 \text{ cm } \%^{-1}$.

source of uncertainty	standard uncertainty /cm
alignment and positioning of plane-parallel chamber	0.05
calibration of vertical translation stage	0.04
beam energy change between measurement and audit (max. 1 % output at $R_{50,dos}$)	0.03
ratio of charge measurements at PDI_{max} and at $PDI_{50\%}$ ($u = 0.1 \%$)	0.003
depth dependent correction for recombination, k_s ($u < 0.1 \%$)	0.003
depth dependent correction for chamber polarity, k_{pol}^+ ($u < 0.1 \%$)	0.003
variation of T and p during a PDI measurement, k_{pT} ($u < 0.2 \%$)	0.006
PDI to PDD conversion [6] ($u = 0.2 \%$)	0.006
combined standard uncertainty, u ($k = 1$)	0.07
expanded uncertainty, U ($k = 2$)	0.14

4.1.2 Uncertainty in a charge measurement at a depth of z_{ref}

Table 4.2 gives the uncertainty budget for the charge measurement procedure, including positioning of an ionization chamber. This uncertainty is used for the D_w measurement and for the cross-calibration of ionization chambers that both take place at a depth of z_{ref} . The uncertainty in SDD is based on (re-)positioning of the water phantom at the desired SSD of 100 cm with an estimated standard uncertainty of 0.10 cm. The uncertainty contribution due to the depth is based on a maximum dose gradient of $-0.4\% \text{ mm}^{-1}$ for 22 MeV at z_{ref} . The uncertainty in determination of z_{ref} based on a measured $R_{50,dos}$ (see Table 4.1) is 0.04 cm and taken into account here. Furthermore, the electrometer calibration, long-term drift and display resolution are taken into account with a combined uncertainty of 0.07%. Uncertainties for the correction of cavity air density are dominated by the thermometer calibration (standard uncertainty, $u = 0.05\text{ °C}$) and the estimated temperature gradient between the ionization chamber and the point where the temperature is measured ($u = 0.10\text{ °C}$) at a nominal water temperature of 20 °C , resulting in a relative standard uncertainty contribution of 0.04%.

Table 4.2: Uncertainty for the determination of a corrected electrometer reading, M_{corr} with an ionization chamber at a depth of z_{ref} , applicable for both plane-parallel and Farmer type cylindrical chambers. Uncertainties in positioning depth are converted to dose with a sensitivity coefficient of $-0.4\% \text{ mm}^{-1}$.

source of uncertainty	standard uncertainty /%
repeated charge measurement (type A)	0.10
SSD ($u = 0.1$ cm at an SDD of 100 cm)	0.20
positioning of ionization chamber in water at z_{ref} ($u = 0.05$ cm)	0.20
electrometer calibration, long term drift and resolution	0.07
k_{pT} : correction for ambient temperature and pressure	0.10
k_h (20% - 80%): variation of relative humidity	0.05
k_S : correction for ion recombination	0.10
k_{pol}^+ : polarity correction	0.10
k_{rn} : variation due to beam radial non-uniformity	0.10
combined standard uncertainty ($k = 1$)	0.37
expanded uncertainty, U ($k = 2$)	0.74

4.1.3 Uncertainty in D_w

Table 4.3 gives the uncertainty budget for a D_w measurement with a plane-parallel Roos chamber calibrated in ^{60}Co . The combined standard uncertainty takes into account the contribution of the corrected electrometer reading, M_{corr} , based on the used measurement procedure (Table 4.2), the uncertainty of the ionization chamber calibration in ^{60}Co and the standard uncertainty in $k_{Q,Q0}$ for the plane-parallel chamber [1]. The uncertainty contribution in $R_{50,\text{dos}}$ as a result of the conversion from PDI to PDD using stopping power ratios is incorporated in the uncertainty of $k_{Q,Q0}$ (see e.g. NCS 18 [1] and IAEA TRS-398 [6]).

Table 4.4 gives the uncertainty budget for D_w in a high-energy electron beam with quality with $R_{50,\text{dos}} > 7$ cm measured with a Farmer type cylindrical ionization chamber calibrated in ^{60}Co . The combined standard uncertainty takes into account the contribution on M_{corr} (Table 4.2), the ^{60}Co calibration and the uncertainty in $k_{Q,Q0}$.

Table 4.5 gives the uncertainty budget for a D_w measurement with a plane-parallel chamber cross-calibrated against a cylindrical chamber in a beam quality Q with $R_{50,\text{dos}} > 7$ cm as indicated in Table 4.4. Except for the uncertainty on the corrected reading of the plane-parallel chamber in beam quality Q , additional uncertainties are two contributions from M_{corr} (Table 4.2) due to the cross-calibration of the plane-parallel chamber against the cylindrical chamber in beam quality Q_{cross} and a contribution for the determination of the plane-parallel chamber's $k_{Q,Q_{\text{cross}}}$.

The expanded uncertainty for a D_w measurement ranges from 2.8 % for a cylindrical chamber in the highest electron energy with $R_{50,\text{dos}} > 7$ cm (Table 4.4), 3.2 % for a cross-calibrated plane-parallel chamber (Table 4.5) to 3.6 % for a plane-parallel chamber calibrated in ^{60}Co (Table 4.3).

Uncertainty contributions indicated with 'audit' in Tables 4.3 to Table 4.5 indicate their contribution to the audit result as explained in the next section.

Table 4.3: Measurement of D_w at a depth of z_{ref} , based on a plane-parallel chamber directly calibrated in ^{60}Co . Uncertainties indicated with 'audit' contribute to the audit result.

source of uncertainty		standard uncertainty /%
M_{corr} : corrected charge measurement at z_{ref} (Table 4.2)	audit	0.37
N_{D,w,Q_0}^{PP} : plane-parallel chamber calibrated in ^{60}Co		0.50
k_{Q,Q_0} : plane-parallel chamber quality correction (NCS 18 [1])		1.70
uncertainty of $R_{50,dos}$ on k_{Q,Q_0} (0.07 cm)	audit	0.09
combined standard uncertainty ($k = 1$)		1.8
expanded uncertainty ($k = 2$)		3.6
combined standard uncertainty contribution to audit result, based on contributions indicated with 'audit' only	audit	0.38

Table 4.4: Measurement of D_w at $R_{50,dos} > 7$ cm, depth of z_{ref} , with a Farmer type cylindrical chamber calibrated in ^{60}Co . Uncertainties indicated with 'audit' contribute to the audit result.

source of uncertainty		standard uncertainty /%
M_{corr} : corrected charge measurement at z_{ref} $R_{50,dos} > 7$ cm (Table 4.2)	audit	0.37
N_{D,w,Q_0}^{CYL} : Farmer type cylindrical chamber calibrated in ^{60}Co		0.50
k_{Q,Q_0} : Farmer chamber beam quality correction (NCS 18 [1])		1.2
uncertainty of $R_{50,dos}$ on cylindrical $k_{Q,cross,Q_0}$ (0.07 cm)	audit	0.09
combined standard uncertainty ($k = 1$)		1.4
expanded uncertainty ($k = 2$)		2.8
combined standard uncertainty contribution to audit result, based on contributions indicated with 'audit' only	audit	0.38

Table 4.5: Measurement of D_w at a depth of z_{ref} , based on a plane-parallel chamber cross-calibrated against a Farmer type cylindrical chamber at beam quality $R_{50,dos} > 7$ cm. Uncertainties indicated with 'audit' contribute to the audit result.

source of uncertainty		standard uncertainty /%
D_w at $R_{50,dos} > 7$ cm with a Farmer type cylindrical chamber (Table 4.4)		1.35
M_{corr} : corrected charge measurement at $R_{50,dos} > 7$ cm (Table 4.2)	audit	0.35
M_{corr} : corrected charge measurement at beam quality Q (Table 4.2)	audit	0.35
$k_{Q,Q_{cross}}$: plane-parallel chamber quality correction (NCS 18 [1])		0.60
influence of measurement of $R_{50,dos}$ on plane-parallel $k_{Q,Q_{cross}}$	audit	0.09
combined standard uncertainty ($k = 1$)		1.6
expanded uncertainty ($k = 2$)		3.2
combined standard uncertainty contribution to audit result, based on contributions indicated with 'audit' only	audit	0.50

4.2 Uncertainties in the audit results

4.2.1 Uncertainty in audit result for $R_{50,dos}$, $\Delta_{R,50,dos}$

The audit result for $R_{50,dos}$ is the difference between the participant's value and the reference value, $\Delta_{R_{50,dos}}$ in the unit cm (see equation (3) section 2.1). Its standard uncertainty $u_{\Delta_{R_{50,dos}}}$ is also expressed in the unit cm and is determined by the quadratic summation of the individual uncertainty contributions of the reference value and the participant's value. Since the participants didn't report uncertainties, their contributing uncertainties are assumed to be at least as high as the uncertainty of the reference value (Table 4.1), i.e. $u_{R,50,dos} = 0.07$ cm. No correlations exist between the $R_{50,dos}$ reference value and participants value. Therefore, the combined uncertainty of the audit result, $U_{\Delta_{R_{50,dos}}}$, is obtained by the quadratic sum of individual uncertainties (i.e. each $U = 0.14$ cm with $k = 2$), resulting in an expanded uncertainty in the audit result:

$$U_{\Delta_{R_{50,dos}}} = 0.20 \text{ cm}$$

4.2.2 Uncertainty in audit result for D_w , $\Delta_{\%,D,w}$

The audit result for D_w is the relative difference between the participant's value and the reference value, Δ_{D_w} in % (see section 2.1). The uncertainty in the audit result for D_w , expressed as $u_{\Delta_{D_w}}$ is also expressed as a relative value and shown in Tables 4.6 until 4.8. Calibration coefficients of the dosimetry equipment of all participants and the NCS-team are traceable to the same calibration laboratory, namely VSL. In addition, the participants and NCS-team apply the same dosimetry protocol (i.e. NCS 18) which uses generic k_Q factors for a certain ionization chamber type. Therefore, the uncertainties on the calibration coefficients and the applied k_Q factors used in the determination of Δ_{D_w} are partially correlated. Since Δ_{D_w} depends on the ratio of the calibration coefficients and the applied k_Q factors, these correlating uncertainties can be partially neglected for the determination of $U_{\Delta_{D_w}}$. Only the uncorrelated part of the uncertainties on the calibration coefficient and the k_Q factor are considered. This is implemented in the calculation of $U_{\Delta_{D_w}}$ in Table 4.5 and 4.6 in the following way. All fully uncorrelated uncertainty contributions to $U_{\Delta_{D_w}}$ are indicated with 'audit' in Tables 4.2 until 4.5 and are transferred to Tables 4.6 to 4.8. For all partially correlated uncertainty contributions (calibration coefficients and k_Q) in Tables 4.2 until 4.5, only the uncorrelated part is added to Tables 4.6 through 4.8 as long-term (<3 year) reproducibility of the

chamber's individual calibration coefficients in ^{60}Co and k_{Q,Q_0} chamber-to-chamber variation for NACP-02 and Roos type chambers respectively.

The magnitude of the plane-parallel chamber-to-chamber variation in k_Q depends on the origin of the calibration coefficient in electron beam quality Q , i.e. calibrated in ^{60}Co or cross-calibrated in a high-energy electron beam (described in section 3.6.2). For plane-parallel chambers calibrated in ^{60}Co the chamber-to-chamber variation is caused by a variation in p_{wall} in ^{60}Co and the uncertainty related to Monte Carlo calculated perturbation corrections, p_Q [1,6]. Due to a lack of information about the uncertainties responsible for chamber-to-chamber variation in k_{Q,Q_0} of well-guarded plane-parallel chambers, in this study an uncertainty contribution of 1.0 % (see Table 4.6) is used. This uncertainty is considered to account for variations of k_{Q,Q_0} between the ionization chamber of the NCS-team and that of the participants.

A similar approach is used with respect to the audit result obtained with a Farmer type cylindrical ionization chamber. However, the chamber-to-chamber variation is smaller due to a better understanding of their perturbation corrections. The uncertainty of the contributing Monte Carlo calculations is 0.77 % [6] for any chamber. The uncertainty contribution as a result of the agreement in k_{Q,Q_0} factors between two Farmer type ionization chambers is estimated to be within 0.50 %.

Tables 4.6 and 4.8 show that the audit result has an expanded uncertainty of 2.4 % ($k = 2$) regardless the method used, i.e. plane-parallel chamber calibrated in ^{60}Co or cross-calibrated in a high-energy electron beam with $R_{50,\text{dos}} > 7$ cm. This is caused by the extra measurements needed to perform the cross-calibration by both institutes which cancels the advantage in smaller uncertainties for beam quality conversion factors.

Not all participants use the same method for D_w determination (some use a plane-parallel chamber calibrated in ^{60}Co others used a cross-calibrated plane-parallel chamber in a high-energy electron beam, Q_{cross}) the uncertainty of the audit result and therefore the expanded uncertainty used in the E_n -score for determination of the audit result (see section 2.2) is taken to be the uncertainty expressed for D_w measurement with plane-parallel chamber for all beam qualities at:

$$U_{\Delta\%,D_w} = 2.4\%$$

Although a distinction could be made between measurements at $R_{50,\text{dos}} > 7$ cm and $R_{50,\text{dos}} \leq 7$ cm, for reason of simplicity of the audit, only one value for the uncertainty is used.

Table 4.6: The uncertainty budget for the audit results $\Delta_{D,w}$ in D_w at beam quality Q with a plane-parallel chamber calibrated in ^{60}Co .

source of uncertainty	standard uncertainty /%
reference D_w value, correlations taken into account (Table 4.3)	0.38
participants D_w value, correlations taken into account (Table 4.3)	0.38
long-term (<3 year) variation of participant's $N_{D,w}$	0.15
k_{Q,Q_0} individual chamber variation for plane-parallel chambers	1.0
combined standard uncertainty ($k = 1$)	1.2
expanded uncertainty ($k = 2$)	2.4

Table 4.7: The uncertainty budget for the audit results $\Delta_{D,w}$ in D_w at beam quality Q with a Farmer type cylindrical chamber in Q_{cross} with $R_{50,\text{dos}} > 7$ cm.

source of uncertainty	standard uncertainty /%
reference D_w value at Q_{cross} , correlations taken into account (Table 4.4)	0.38
participants D_w value at Q_{cross} , correlations taken into account (Table 4.4)	0.38
long-term (<3 year) variation of participant $N_{D,w}$	0.15
k_{Q,Q_0} individual chamber variation for cylindrical chambers	0.50
combined standard uncertainty ($k = 1$)	0.75
expanded uncertainty ($k = 2$)	1.5

Table 4.8: The uncertainty budget for the audit results $\Delta_{D,w}$ in D_w at beam quality Q with a plane-parallel chamber cross-calibrated in Q_{cross} with $R_{50,\text{dos}} > 7$ cm.

source of uncertainty	standard uncertainty /%
reference D_w value at Q_{cross} , correlations taken into account (Table 4.4)	0.38
participants D_w value at Q_{cross} , correlations taken into account (Table 4.4)	0.38
long-term (<3 year) variation of participant $N_{D,w}$ for cylindrical in ^{60}Co	0.15
k_{Q,Q_0} individual chamber variation for cylindrical chambers	0.50
reference D_w value at Q, correlations taken into account (Table 4.5)	0.50
participants D_w value at Q, correlations taken into account (Table 4.5)	0.50
k_{Q,Q_0} individual chamber variation for plane-parallel chambers	0.50
combined standard uncertainty ($k = 1$)	1.2
expanded uncertainty ($k = 2$)	2.4

5 Results

5.1 Reference and participants' values

Table 5.1 gives the reference and participant's values for $R_{50,dos}$ and D_w during the audit measurements at the participants sites. For completeness the reference depth, z_{ref} , is reported. The D_w reference value is based on measurement with the plane-parallel chamber both calibrated in ^{60}Co (column indicated with D_w) according to 3.6.1 and based on a cross-calibration in a high-energy electron beam (column indicated with D_w^{**}) according to section 3.6.2. The uncertainties are 3.6 % and 3.2 % ($k = 2$), as respectively reported in table 4.3 and table 4.5 of section 4.2.

Table 5.1: Reference values and participants' values during the audit. Values indicated with ** are based on a cross-calibration of a plane-parallel chamber in a high-energy electron beam.

site (see Table 1.1)	date (2015)	E /MeV	reference value				participants' value		
			$R_{50,dos}$ /cm	z_{ref} /cm	D_w /cGy	D_w^{**} /cGy	$R_{50,dos}$ /cm	z_{ref} /cm	D_w /cGy
AVL	16/07	6	2.54	1.42	199.4	197.6	2.63	1.48	198.4**
		12	4.88	2.83	200.8	198.9	4.99	2.89	199.7**
		18	7.20	4.22	197.1	195.3	7.35	4.31	196.1**
RdG	30/07	4	1.62	0.87	197.1	-	1.60	0.86	197.3
		10	3.99	2.29	196.0	-	4.00	2.30	196.8
		15	6.00	3.50	196.0	-	6.27	3.66	195.6
VUmc	25/08	6	2.39	1.34	304.8	305.8	2.38	1.33	304.8**
		9	3.63	2.08	296.1	297.0	3.60	2.06	296.9**
		22	8.75	5.15	286.5	287.4	8.78	5.17	286.8**
LUMC	15/09	4	1.61	0.86	199.3	-	1.60	0.86	199.6
		12	4.64	2.69	200.0	-	4.78	2.77	199.3
		12	4.64	2.69	200.0	-	4.78	2.77	199.3
AVL	05/11	6	2.55	1.43	199.6	199.4	2.51	1.41	198.7**
		12	4.93	2.86	198.8	198.6	4.95	2.87	197.4**
		18	7.22	4.24	197.4	197.2	7.32	4.29	195.4**

* High Dose Rate Electron beam (HDRE) with the application of NCS 18 [1] at a field size of $40 \times 40 \text{ cm}^2$.

**Value(s) obtained via a cross-calibration of a plane-parallel chamber against a farmer chamber in a high-energy electron beam according to section 3.6.2.

5.2 Audit results

Table 5.2 and Figures 5.1 and 5.2 give the audit results for the participants in this study. Audit results are based on a reference value with the plane-parallel chamber both calibrated

in ^{60}Co (column indicated with Δ_{D_w}), see section 3.6.1, and based on a cross-calibration in a high-energy electron beam (column indicated with $\Delta_{D_w}^{**}$), see section 3.6.2. The uncertainties on both audit results are both 2.4 % ($k=2$) as respectively reported in Table 4.6 and Table 4.8 of section 4.2.

The audit results indicated 'satisfactory' or 'unsatisfactory' in the final column are based on the analyses of the E_n -scores. E_n -scores for D_w measurement range between 0.0 and 0.6 show excellent agreement. Based on these E_n -scores at all 15 beam qualities between 4 MeV and 22 MeV, it can be concluded that the audit results for the D_w measurements of all institutes were 'satisfactory'.

Table 5.2 and the Figures 5.1 and 5.2 also show that only one of the E_n -scores for $R_{50,dos}$ is > 1 . All other 14 audit measurements for $R_{50,dos}$ resulted in a satisfactory E_n -score. It should be noted that despite the fact that one of the results for $R_{50,dos}$ might be qualified as 'unsatisfactory', its value is within $k=3$ (99 % coverage interval and corresponding to 0.21 cm) from the reference value.

The audit results (Figure 5.1 and Table 5.2) show a noticeable difference of about 1 % between the ^{60}Co and cross-calibrated reference values during the first audit (AVL 16/07). This difference is not present during the final audit (AVL 05/11), conducted at the same institute. The difference between ^{60}Co and cross-calibrated values are about 0.1 % instead. Additionally, both audits show equal E_n -scores on the audit result.

Table 5.2: Audit results for $R_{50,dos}$ and D_w in 15 electron beams at the 4 participating institutes of this study.

Site (see Table 1.1)	date (2015)	E /MeV	$R_{50,dos}$		D_w				PT result
			$\Delta_{R_{50,dos}}$ /cm	E_{n^-} score	Δ_{D_w} /%	E_{n^-} score	$\Delta_{D_w}^{**}$ /%	E_{n^-} score	
AVL	16/07	6	0.09	0.5	-0.52	0.2	0.40	0.2	satisfactory
		12	0.11	0.6	-0.51	0.2	0.42	0.2	satisfactory
		18	0.15	0.8	-0.55	0.2	0.38	0.2	satisfactory
RdG	30/07	4	-0.02	0.1	0.09	0.0	-	-	satisfactory
		10	0.01	0.1	0.42	0.2	-	-	satisfactory
		15	0.27	1.4	-0.20	0.1	-	-	satisfactory
VUmc	25/08	6	-0.01	0.1	0.02	0.0	-0.30	0.1	satisfactory
		9	-0.03	0.2	0.28	0.2	-0.04	0.0	satisfactory
		22	0.03	0.2	0.08	0.0	-0.23	0.1	satisfactory
LUMC	15/09	4	-0.01	0.1	0.14	0.1	-	-	satisfactory
		4 HDRE*	0.02	0.1	0.90	0.4	-	-	satisfactory
		12	0.14	0.7	-0.39	0.2	-	-	satisfactory
AVL	05/11	6	-0.03	0.2	-0.43	0.2	-0.34	0.1	satisfactory
		12	0.02	0.1	-0.69	0.3	-0.59	0.3	satisfactory
		18	0.10	0.5	-1.0	0.4	-0.94	0.6	satisfactory

* High Dose Rate Electron beam (HDRE) with the application of NCS 18 [1] at a field size of $42 \times 42 \text{ cm}^2$, which is larger than the surface of the audit phantom,

**Value(s) obtained via a cross-calibration of a plane-parallel chamber against a farmer chamber in a high-energy electron beam according to section 3.6.2.

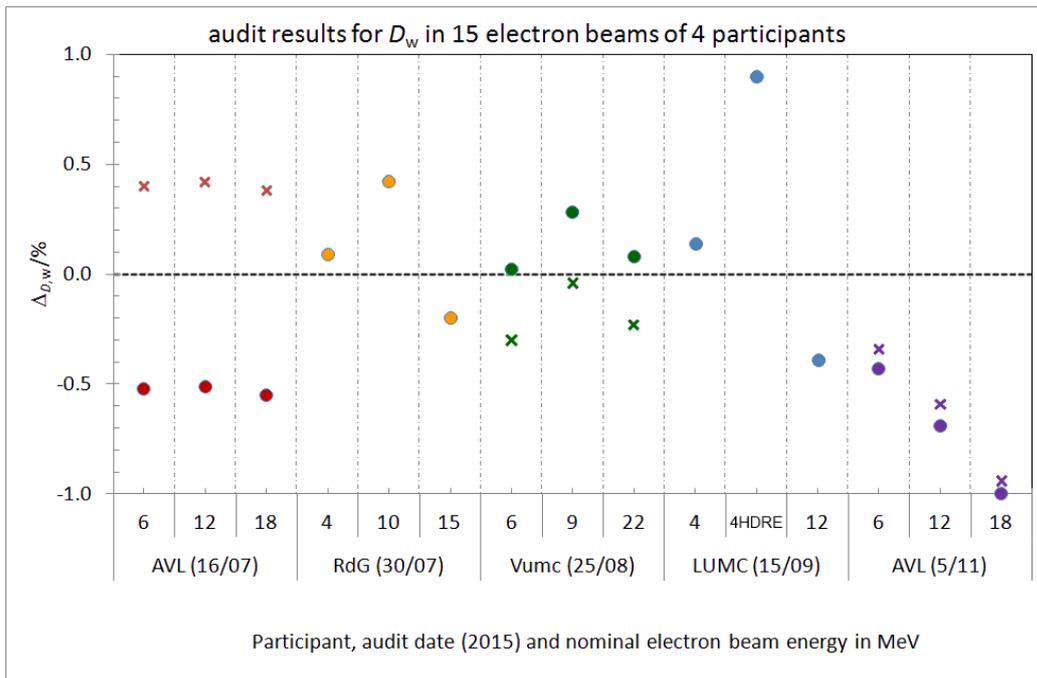


Figure 5.1: Audit results for $R_{50,dos}$ in the 15 electron beams of the 4 participants. The dotted line through $\Delta_{D,w} = 0.0\%$ represents the reference value. Circles and crosses respectively indicate reference values based on a plane-parallel chamber calibrated in ^{60}Co and cross-calibrated in a high-energy electron beam.

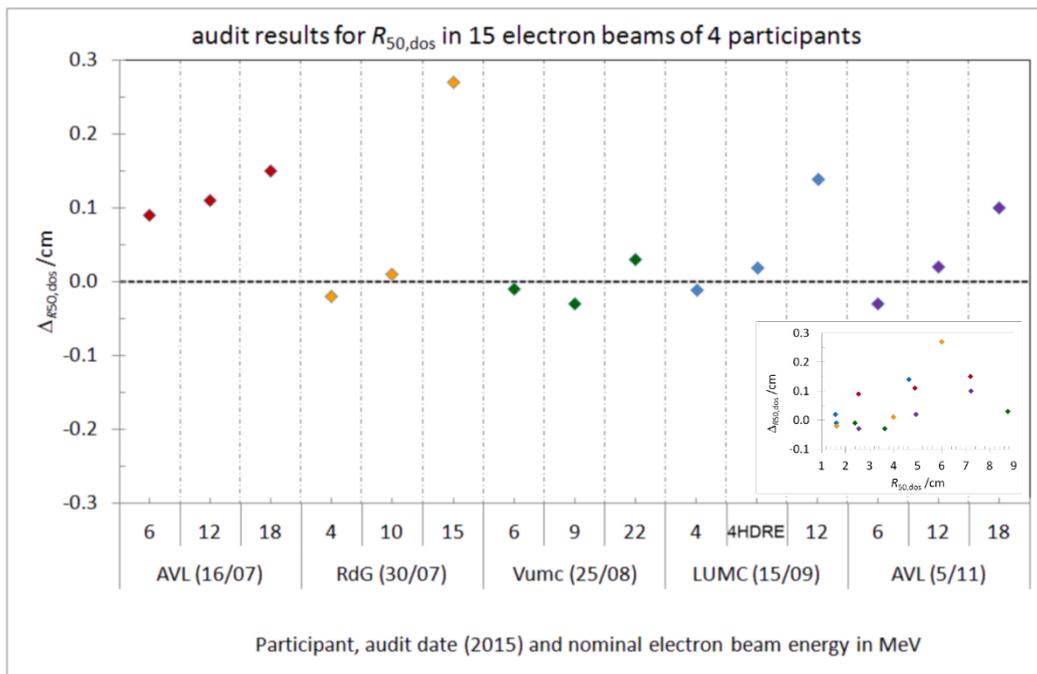


Figure 5.2: Audit results for D_w in the 15 electron beams of the 4 participants and as a function of $R_{50,dos}$ (bottom-right inset).

6 Discussion and conclusion

During this study, a total of 15 electron beams were measured in 4 participating institutes. One institute was measured twice, i.e. at the beginning of the audit campaign as an initial test audit and at the end of the audit campaign as an actual audit. Both results have been reported.

All $R_{50,dos}$ audit results, $\Delta_{R_{50,dos}}$, turned out to be satisfactory (i.e. $|E_n| \leq 1.0$) except for one electron beam with an unsatisfactory E_n -score of 1.4. Besides that, this value still agreed within 3 standard uncertainties, it did not influence the audit result on the D_w measurement and therefore the overall audit result of this participant.

All D_w audit results, Δ_{D_w} , turned out to be satisfactory (i.e. $|E_n| \leq 1.0$) regardless the choice of calibration method for the plane-parallel chamber (i.e. ^{60}Co -calibrated or cross-calibrated in a high-energy electron beam). However, at the first (test) audit a discrepancy of 1 % was found between D_w values based on the ^{60}Co -calibration compared to its cross-calibration based value. Since the ^{60}Co -based value of the first audit was consistent with both ^{60}Co -based and cross-calibration based values of the final audit at the same department, it was concluded that the cross-calibration of the NCS audit team at the first (test) audit was incorrect. The error is expected to be caused by the lack of experience in use of the NCS-equipment; more specifically misalignment of the Farmer type cylindrical chamber at the reference depth. This was confirmed by the ^{60}Co -based value at the beam quality which was consistent with the value measured at the final audit.

With respect to the uncertainty for the determination of absorbed dose under reference conditions, the smallest uncertainty of 2.8 % is achieved with a Farmer type cylindrical chamber in a high-energy electron beam with $R_{50,dos} > 7$ cm (Table 4.4). Generally, for all electron beam qualities, the smallest uncertainty of 3.2 % is achieved with a cross-calibrated plane-parallel chamber against a Farmer chamber in a high-energy electron beam when this calibration is performed with care (Table 4.5). The third option, however a much simpler and time efficient measurement, is to obtain D_w with a plane-parallel chamber calibrated in ^{60}Co and results in an uncertainty of 3.6 % (Table 4.3).

In this study the uncertainty on the audit result based on a ^{60}Co calibrated plane-parallel chamber or a cross-calibrated plane-parallel chamber was estimated to be equal, i.e. 2.4 %, when care is taken performing the cross-calibration (Table 4.6 and Table 4.8). Although a distinction could be made for the audit results above $R_{50,dos} > 7$ cm with a smaller standard uncertainty of 1.5 % (Table 4.7) for reason of simplicity of the audit, a single uncertainty value of 2.4 % was used.

It should be noted that the audit described in this study, was performed at radiotherapy departments that are using measurement instruments traceable to VSL and that are applying the same code of practice as the NCS audit team. If this audit would be performed at a department that uses measurement equipment not traceable to VSL or applies a different dosimetry protocol than the NCS audit team, the uncertainties reported in this study would not apply.

Overall it can be concluded that the audit has been implemented successfully. Differences of D_w values between the audit team and the participant were in all cases smaller than 1 % and in most cases smaller than 0.5 % with a relative uncertainty of 2.4 % ($k = 2$). Differences in $R_{50,dos}$ were in all cases smaller than 0.3 cm and in most cases smaller than 0.2 cm with an uncertainty of 0.20 cm. Except for the first (test) audit, D_w values obtained with a plane-parallel chamber calibrated in ^{60}Co agreed within 0.3 % with D_w values obtained with plane parallel chambers cross-calibrated in a high-energy electron cross-calibration.

7 Acknowledgements

The subcommittee would like to thank Wenze van Klink for his work for the subcommittee as member during his employment at the VU Medical Center.

References

- [1] Aalbers AHL, Hoornaert M-T, Minken A, Palmans H, Pieksma MWH, De Prez LA, Reynaert N, Vynckier S, Wittkämper FW, NCS Report 18: Code of practice for the absorbed dose determination in high energy photon and electron beams, Delft, 2008. doi:10.25030/ncs-018.
- [2] Perik TJ, De Prez LA, Aalbers AHL, Monseux A, Sergent F, Wittkämper FW, Van de Kamer JB, NCS Report 23: Audit of high-energy photon beams in Belgian and Dutch radiotherapy departments, Delft, 2013. doi:10.25030/ncs-023.
- [3] ISO/IEC, Conformity assessment - General requirements for proficiency testing (ISO/IEC 17043:2010, IDT), Geneva, 2010.
- [4] Mijnheer BJ, Aalbers AHL, Van Gasteren JJM, Visser AG, Wittkämper FW, NCS Report 2: Code of practice for the dosimetry of high-energy photon beams, Delft, 1986. doi:10.25030/ncs-002.
- [5] Wittkämper FW, Aalbers AHL, Brouwer WFM, Huizenga H, Mijnheer BJ, Piron AJ, Vynckier S, NCS Report 5: Code of practice for the dosimetry of high-energy electron beams, Delft, 1989. doi:10.25030/ncs-005.
- [6] Andreo P, Burns DT, Hohlfield K, Huq MS, Kanai T, Laitano F, Smyth VG, Vynckier S, IAEA TRS-398: Absorbed Dose Determination in External Beam Radiotherapy, International Atomic Energy Agency, Vienna, 2006.
- [7] Thwaites DI, Burns DT, Klevenhagen SC, Nahum AE, Pitchford WG, The IPEMB code of practice for electron dosimetry for radiotherapy beams of initial energy from 2 to 50 MeV based on an air kerma calibration, *Phys. Med. Biol.* 41 (1996) 2557–2603. doi:10.1088/0031-9155/41/12/001.
- [8] Zink K, Czarnecki D, Looe HK, von Voigts-Rhetz P, Harder D, Monte Carlo study of the depth-dependent fluence perturbation in parallel-plate ionization chambers in electron beams, *Med. Phys.* 41 (2014) 111707. doi:10.1118/1.4897389.
- [9] Weinhaus MS, Meli JA, Determining Pion, the correction factor for recombination losses in an ionization chamber., *Med. Phys.* 11 (1984) 846–849. doi:10.1118/1.595574.
- [10] Bichsel H, Pierson DH, Boring JW, Green A, Inokuti M, Hurst G, ICRU report 31: Average Energy Required to Produce an Ion Pair, Washington D.C., 1979. doi:10.1017/CBO9781107415324.004.
- [11] JCGM, Evaluation of measurement data: Guide to the expression of uncertainty in measurement, Bureau International des Poids et Mesures, 2008. doi:10.1373/clinchem.2003.030528.

